




1000 V Direct Input Multi-channel Logger

- **As a Multichannel Logger**
The MR8875 delivers multichannel measurement capability in a compact, A4-size footprint that ensures easy portability. Depending on which input modules are installed, measurement capabilities range from 16 analog channels to 60 thermocouple temperature measurement channels.
- **As a Super-High-Speed Logger**
The MR8875 can simultaneously sample all channels in as little as 2 μsec .
Sample up to 2 channels in 2 μsec or up to 60 channels in 50 μsec while writing data continuously to an SD memory card in real time. * Operation is guaranteed only with a genuine Hioki SD memory card.
- **As a Long-Term Continuous Recording Logger**
Real-time saving to SD card
At an interval of 100 msec, the MR8875 can record 8 channels of data for 155 days or 60 channels of data for 20 days. * Operation is guaranteed only with a genuine Hioki SD memory card.
- **Introducing a new input module that accepts up to 1000 V input and measures in RMS**
Select and install four input modules from a large selection. The MR8875 lets you mix and match modules to measure voltage, temperature, strain, and CAN signals or measure sensor output signals at a high, 16-bit resolution.

User-selectable input modules for more applications! A compact solution for multichannel measurement

Industrial Robots

Voltage Temperature Control Signals Strain

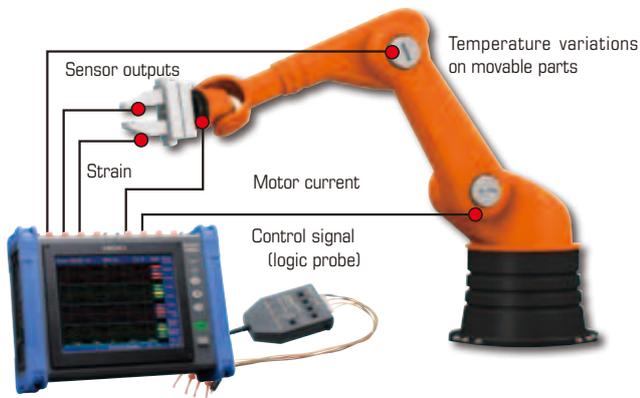

The plug-in module-based architecture means you can mix and record a variety of signals across multiple channels - ideal for verifying the operation of multi-axis robots.

Example of module combinations

Analog Unit MR8901	× 2
Voltage/Temp Unit MR8902	× 1
Strain Unit MR8903	× 1

R&D or Science Experiments

Voltage Temperature



With its multichannel, long-term recording capabilities, the **MR8875** is ideally suited for use in development applications such as performance and durability testing.

- Record sensor output.
- Evaluate sensors and other devices.
- Use as an X-Y recorder (flatbed).

Example of module combinations

Analog Unit MR8901	× 2
Voltage/Temp Unit MR8902	× 2

Development of Construction Machinery, Agricultural Machinery, and Automobiles

Voltage Temperature Strain



Enhanced environmental temperature and vibration resistance enable the **MR8875** to withstand harsh measurement environments.

Example of module combinations

Analog Unit MR8901	× 1
Voltage/Temp Unit MR8902	× 1
Strain Unit MR8903	× 1
CAN Unit MR8904	× 1


Applications

High-speed Data Recorder MR8875

For inverter and motor testing

High-voltage input (MR8905)

Primary- and secondary-side measurement of UPS power supply and commercial power supply transformers
Record inverter primary- and secondary-side waveforms

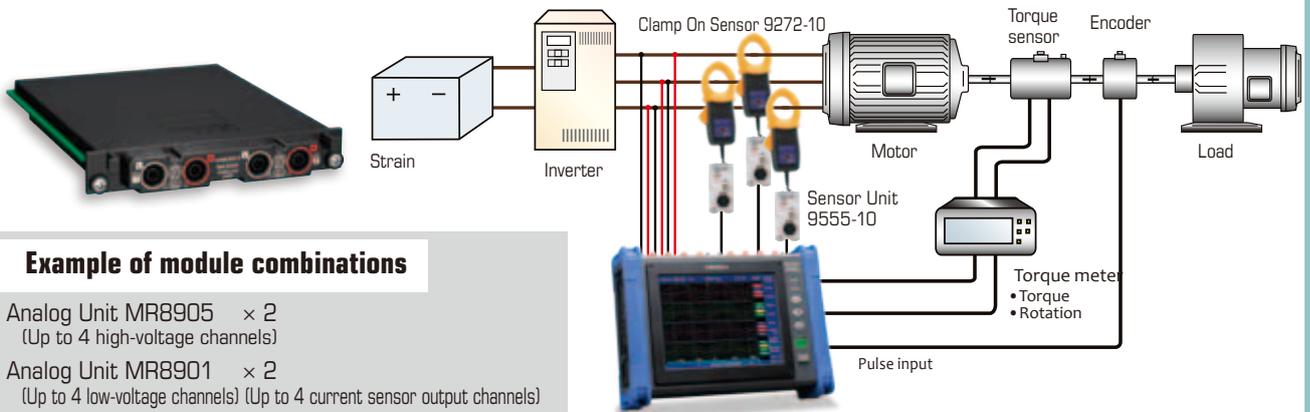

Example of module combinations



- Analog Unit MR8905 × 2
(Up to 4 high-voltage channels)
- Analog Unit MR8901 × 2
(Up to 4 low-voltage channels) (Up to 4 current sensor output channels)

Testing of EV batteries

1000 V DC (CAT II)

Measure ECU and EV inverter output waveforms

With the MR8905 Analog Unit, the MR8875 can measure the voltage of individual battery cells—a process that requires high precision and high resolution—at 16 bits of resolution (1/1250 of the range). The instrument can measure signals of up to 1000 V DC directly.

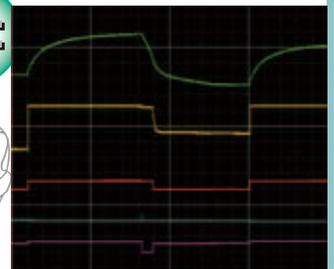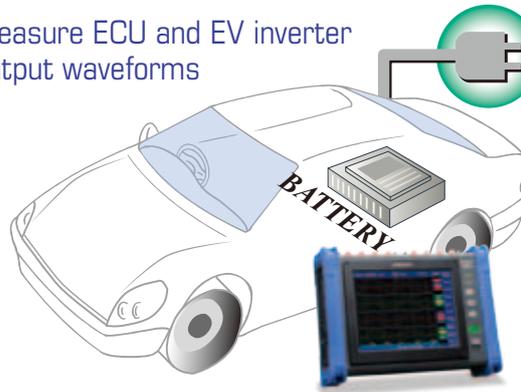


- Battery evaluation
(Example of control signal and charge/discharge time measurement)

Testing of power equipment

600 V AC (CAT III)

Characteristics testing of power equipment (Load rejection and circuit breaker testing)

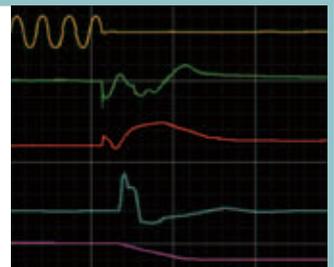

- Load rejection testing
Analyze the correlations among factors such as the generator voltage before and after circuit-breaker operation, degree of variability in RPM, governor servo operating status, and pressure regulator operation timing.

1 Real-Time Saving to SD Card in High Resolution

Collect physical signals at a 500 kS/s sampling rate with a high resolution of 25,000 points f.s.

The same working principle as that of a digital oscilloscope is used to record data to the large-capacity internal memory at high speed. The sampling rate is 500 kS/s (2 μs period) on all channels simultaneously. Sensor signal waveforms are recorded and represented faithfully. Furthermore, a 16-bit A/D resolution ensures even subtle changes in the sensor signals are not missed.

Internal memory
8MW/unit


Ultra-high speed SD data recorder is a vast improvement over legacy products

The MR8875 takes advantage of revolutionary SD card technologies to offer faster real-time saving to a memory card from as fast as 2 μs intervals (operation is guaranteed only with a genuine HIOKI SD memory card). When the recording period (sampling rate) is 50 μs or less, data for all 60 channels can be recorded continuously over a long period.



Maximum recordable time to an 2GB SD memory card


- * Since the header information is included, actually recordable measurement data is approximately 90% of the times shown in the table below. The upper limit is 1,000 days but operation is guaranteed for 1 year.
- * The recording interval is limited depending on the number of measurement ON channels.
- * Built-in logic, pulses P1 and P2 each use the capacity equivalent to one analog channel.

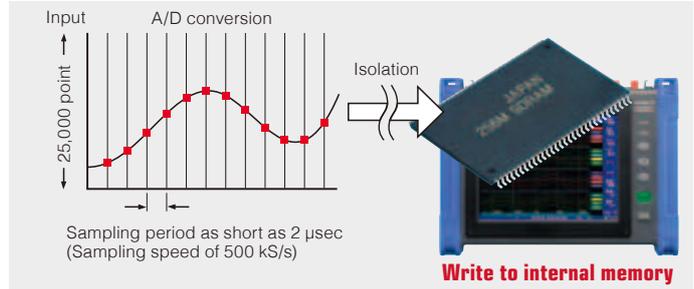

Maximum time to record to the internal storage memory (Abridged)

- * The maximum number of channels to be used is 16 because memory for recording to the internal memory is allocated to each input module.
- * Built-in logic, and pulses P1 and P2 each use the capacity equivalent to one analog channel.

Time axis (Abridged)	Sampling	No. of channels to be used		
		1 ch	3 to 4 ch	9 to 16 ch
200 μs/div	2 μs	80,000div	20,000div	5000div
1 ms/div	10 μs	16 s	4s	1s
10 ms/div	100 μs	1 min 20 s	20s	5s
100 ms/div	1 ms	13 min 20 s	3min 20s	50s
1 s/div	10 ms	2 h 13 min 20 s	33min 20s	8min 20s
10 s/div	100 ms	22 h 13 min 20 s	5h 33min 20s	1h 23min 20s
100 s/div	1.0 s	9 d 06 h 13 min 20 s	2d 07h 33min 20s	13h 53min 20s
5 min/div	3.0 s	277d 18h 40min	69d 10h 40min	17d 08h 40min

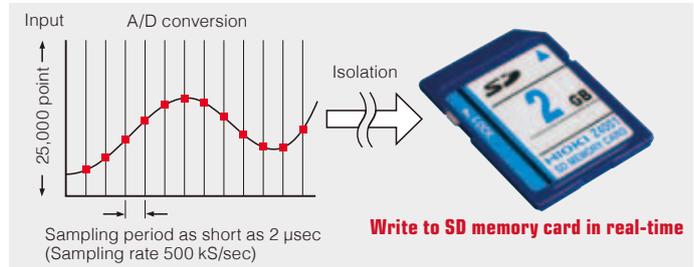

Time axis	Recording intervals	1 ch	2 ch	4 ch	8 ch	16 ch	30 ch	60 ch
200 μs/div	2 μs	35 min 47 s	17 min 53 s	Not applicable				
500 μs/div	5 μs	1 h 29 min 28 s	44 min 44 s	22 min 22 s	11 min 11 s	Not applicable	Not applicable	Not applicable
1 ms/div	10 μs	2 h 58 min 57 s	1 h 29 min 28 s	44 min 44 s	22 min 22 s	11 min 11 s	Not applicable	Not applicable
2 ms/div	20 μs	5 h 57 min 54 s	2 h 58 min 57 s	1 h 29 min 28 s	44 min 44 s	22 min 22 s	11 min 55 s	Not applicable
5 ms/div	50 μs	14 h 54 min 47 s	7 h 27 min 23 s	3 h 43 min 41 s	1 h 51 min 50 s	55 min 55 s	29 min 49 s	14 min 54 s
10 ms/div	100 μs	1 d 05 h 49 min 34 s	14 h 54 min 47 s	7 h 27 min 23 s	3 h 43 min 41 s	1 h 51 min 50 s	59 min 39 s	29 min 49 s
20 ms/div	200 μs	2 d 11 h 39 min 08 s	1 d 05 h 49 min 34 s	14 h 54 min 47 s	7 h 27 min 23 s	3 h 43 min 41 s	1 h 59 min 18 s	59 min 39 s
50 ms/div	500 μs	6 d 05 h 07 min 50 s	3 d 02 h 33 min 55 s	1 d 13 h 16 min 57 s	18 h 38 min 28 s	9 h 19 min 14 s	4 h 58 min 15 s	2 h 29 min 07 s
100 ms/div	1 ms	12 d 10 h 15 min 41 s	6 d 05 h 07 min 50 s	3 d 02 h 33 min 55 s	1 d 13 h 16min 57 s	18 h 38 min 28 s	9 h 56 min 31 s	4 h 58 min 15 s
200 ms/div	2 ms	24 d 20 h 31 min 23 s	12 d 10 h 15 min 41 s	6 d 05 h 07 min 50 s	3 d 02 h 33 min 55 s	1 d 13 h 16 min 57 s	19 h 53 min 2 s	9 h 56 min 31 s
500 ms/div	5 ms	62 d 03 h 18 min 29 s	31 d 01 h 39min 14 s	15 d 12 h 39 min 14 s	7 d 18 h 24 min 48 s	3 d 21 h 12 min 24 s	2 d 01 h 42 min 36 s	1 d 00 h 51min 18 s
1 s/div	10 ms	124 d 06 h 36 min 58 s	62 d 03 h 18 min 29 s	31 d 01 h 39 min 14 s	15 d 12 h 49 min 37 s	7 d 18 h 24 min 48 s	4 d 03 h 25 min 13 s	2 d 01 h 42 min 36 s
2 s/div	20 ms	248 d 13 h 13 min 56 s	124 d 06 h 36 min 58 s	62 d 03 h 18 min 29 s	31 d 01 h 39 min 14 s	15 d 12 h 49 min 37 s	8 d 06 h 50 min 27 s	4 d 03 h 42 min 36 s
5 s/div	50 ms	621 d 09 h 04 min 51 s	310 d 16 h 32 min 25 s	155 d 08 h 16 min 12 s	77 d 16 h 08 min 06 s	38 d 20 h 04 min 03 s	20 d 17 h 06 min 09 s	10 d 08 h 33 min 04 s
10 s/div	100 ms	Upper limit 1000 days	621 d 09 h 04 min 51 s	310 d 16 h 32 min 25 s	155 d 08 h 16 min 12 s	77 d 16 h 08 min 06 s	41 d 10 h 12 min 19 s	20 d 17 h 06 min 09 s
30 s/div	300 ms	Upper limit 1000 days	Upper limit 1000 days	932 d 01 h 37 min 16 s	466 d 00 h 48 min 38 s	233 d 00 h 24 min 19 s	124 d 06 h 36 min 58 s	62 d 03 h 18 min 29 s
50 s/div	500 ms	Upper limit 1000 days	Upper limit 1000 days	Upper limit 1000 days	776 d 17 h 21 min 04 s	388 d 08 h 40 min 32 s	207 d 03 h 01 min 37 s	103 d 13 h 30 min 48 s
60 s/div	600 ms	Upper limit 1000 days	Upper limit 1000 days	Upper limit 1000 days	932 d 01 h 37 min 17 s	466 d 00 h 48 min 38 s	248 d 13 h 13 min 56 s	124 d 06 h 36 min 48 s
100 s/div	1.0 s	Upper limit 1000 days	776 d 17 h 21 min 04 s	414 d 06 h 03 min 14 s	207 d 03 h 01 min 37 s			
2 min/div	1.2 s	Upper limit 1000 days	932 d 01 h 07 min 17 s	497 d 02 h 27 min 53 s	248 d 13 h 13 min 56 s			
5 min/div	3.0 s	Upper limit 1000 days	621 d 09 h 04 min 51 s					

2 Multichannel Mixed Measurement of Various Signals

Install input modules according to your specific needs

- The **MR8875** uses a plugin unit-type input amp setup that allows users to select the input unit that's appropriate for their measurement objective. In addition, it's easy to change input units after purchase.
- The Analog Unit **MR8905**, which can accommodate high voltages and which allows direct input of up to 1,000 V (CAT II) or 600 V (CAT III), is available for high-voltage applications. In addition to instantaneous waveforms, measurement of RMS level waveforms is also supported (starting with Ver. 2.14/3.14 of the **MR8875**).
- Even the standard input unit supports 1,000 V (CAT III) measurement if used with the newly developed Differential Probe P9000 series of small probes.
- For high-sensitivity measurement, use the Strain Unit **MR8903**, which features 1 mV f.s. operation (for a maximum resolution of 0.04 μ V). Measurement of minuscule sensor output is also supported.



Recorder accepts direct pulse input or standard logic probe terminals

The **MR8875** offers two standard pulse input channels that allow for inputting no-voltage a- and b-contacts, open collector, or voltage. Signals transmitted as pulses, such as those of rotation number and flow rate, can be measured or counted. Use a logic probe for the ON/OFF (logic) signal waveforms of a relay and PLC. Two types of logic probes are available depending on the signal format.



Support for a wide variety of measurement items

(Model MR8875 ships standard with pulse input capability. Logic input requires optional logic probe.)


Measurement target	Input unit	Measurement range	Resolution	Sampling	Frequency characteristics
Rotation	Standardly equipped with pulse input	5000 (r/s) f.s.	1 (r/s)	10 msec (100 S/s)	N/A
Pulse totalization	Standardly equipped with pulse input	65,535 to 3,276,750,000 counts f.s.	1 count	N/A	N/A
Relay contacts, voltage on/off	Logic Probe 9320-01	Depends on logic probe in use * Max. input 50 V, threshold +1.4/+2.5/+4.0 V * Non-voltage contact, short/open	N/A	2 μ sec (500 kS/s)	500 nsec or lower response
AC/DC voltage on/off	Logic Probe MR9321-01	Depends on logic probe in use * Detect presence of AC/DC voltages of up to 250 V.	N/A	2 μ sec (500 kS/s)	3 msec or lower response

Note: Power line frequency, duty ratio and pulse width measurements are not supported.



MR8905

The Analog Unit MR8905 does not include input cables. Separate purchase of the optional Connection Cable Set L4940 (x 2) and Alligator Clip Set L4935 (x 2), which consists of clips that fit onto the ends of the cables, is required.

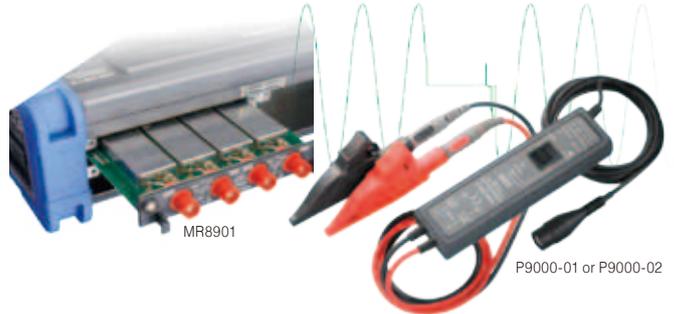

MR8901

P9000-01 or P9000-02

The Differential Probe P9000 can be used with the standard Analog Unit MR8901 to enable high-voltage, 1,000 V (CAT III) measurement. The P9000-02 further enables RMS level measurement of AC power lines.



• Example of instrument recording the instantaneous waveform and RMS level waveform during a momentary outage of an AC power supply (using the MR8905)




• Multi-channel timing measurement using logic waveform measurement

Pulse input terminal

Take advantage of the frequency dividing function, settable from 1 to 50,000 counts, to take direct readings from an encoder that outputs multi-point pulses according to the rotation number.



Two line pulse inputs (Common GND)

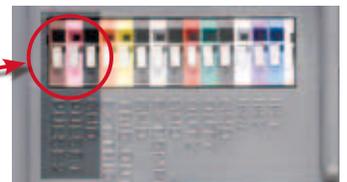

3 Touch Screen for Intuitive Operation


Touch screen interface improves operating efficiency

Buttons on the MR8875 are kept to a minimum by utilizing touch screen technology. The high-definition 8.4-inch high-brightness TFT color LCD is the interface of choice for improving productivity by offering a more intuitive experience than traditional input methods. While the connection terminals are located at the top panel of the MR8875, when cables need to be connected from the bottom, simply swipe the screen from top to bottom at either edge and the screen will rotate correspondingly. The MR8875 can be set in a position that is easier to use according to the installation location.



Touch to scroll back or scale the waveform

Display earlier waveforms during recording without stopping measurement by simply touching the scroll icons on the screen. You can also scale the waveform amplitude by just swiping through the waveform up (to zoom in) or down (to zoom out).

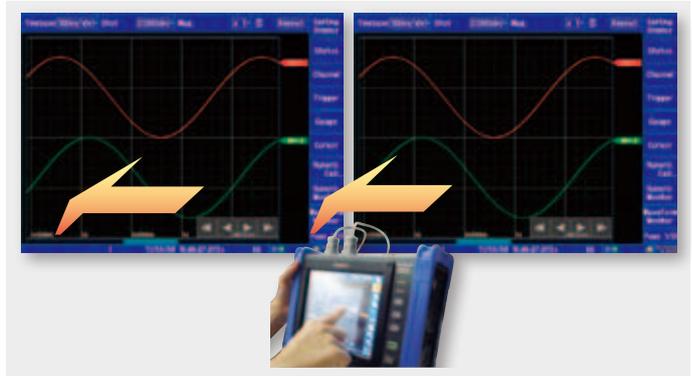


Advanced cursor read function for multichannel analysis

Six cursors A, B, C, D, E, and F are available, compared with the conventional A- and B-cursors.

Use the cursors to measure and display the following:


- A, B, C, and D: Potential and time from the trigger
- E and F: Potential
- A-B and C-D cursors: Time difference and potential difference
- E-F cursors: Potential

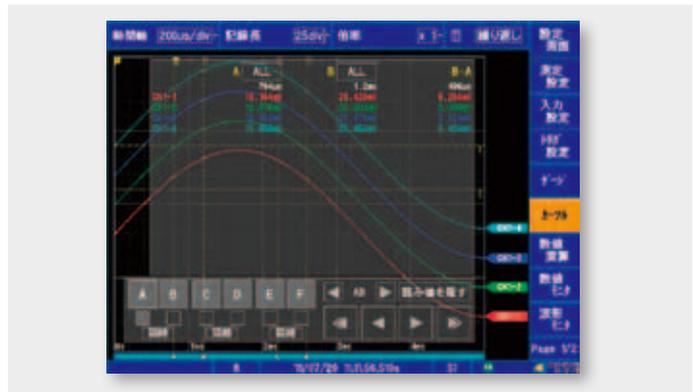

Split screen, sheet display, event mark input, and jump functions indispensable for efficient analysis

Split screen and sheet display functions are provided to support multiple channels. Individual display formats can be selected and an application can be assigned to each sheet for analysis, increasing productivity.

★ For long-term recordings, tag important points with event markers. Up to 1000 markers can be placed so that you can quickly jump to them later for detailed analysis.

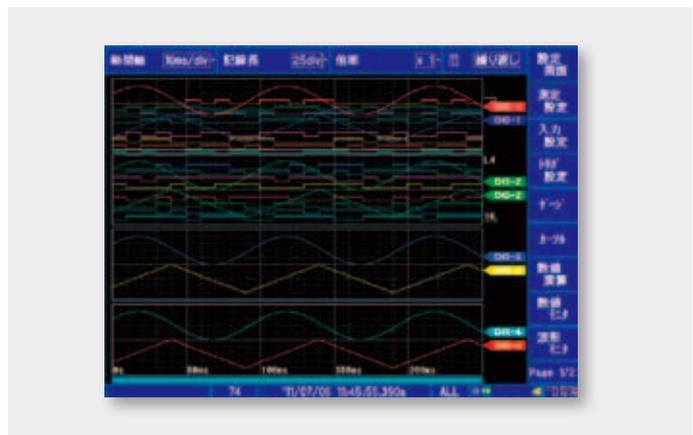


4 Computer Analysis via LAN, SD, and USB memory interfaces

LAN-compatible Web/FTP server function and waveform/CSV conversion using supplied standard software Wv

Take advantage of the built-in 100BASE-TX LAN interface to network with the PC:

<WEB server> Use the Web Server function to view waveforms and remotely control the **MR8875** with your PC's web browser

<FTP server> Use the FTP server function to copy the data stored in memory (SD card, USB memory, or internal storage memory) to the PC. View waveforms for binary data acquired with the **MR8875** on a PC, or convert data to CSV using the free WaveViewer (Wv) application for further analysis in Excel. Download the latest version of the WaveViewer from the HIOKI website at www.hioki.com.

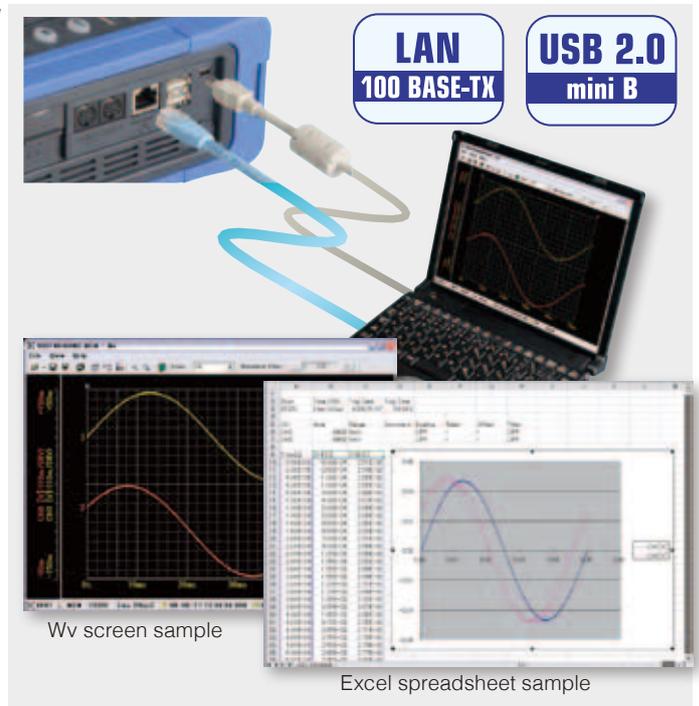

Remotely control the MR8875 using the Web server function


Use a typical web browser to see the screen of the **MR8875** on your PC with no other special software

required. Make settings, acquire data, and monitor the screen with ease.

Note: Waveform data cannot be acquired from the internal memory during measurement.

Transfer data using FTP

After measurement is finished, data is transferred automatically to the FTP server that is running on the PC. Data can also be transferred manually.

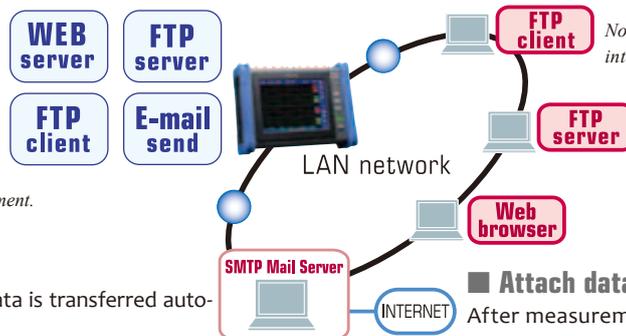

Download data using FTP

Measurement data in files on recording media and in the internal memory can be acquired from a PC.

Note: Waveform data cannot be acquired from the internal memory during measurement.

Attach data to E-mail

After measurement is finished, you can automatically send the captured data as an e-mail attachment. Data can also be transferred manually.

Save data to the USB memory or SD card

Convenient USB memory*1 or SD memory cards can be used to copy data stored in the internal storage memory to the PC. Data stored in the **MR8875**'s SD card can also be downloaded to the PC using a USB cable.*2

*1 Data can be saved to USB memory. However, it is recommended to use a genuine Hioki SD card for which operation is guaranteed to ensure data protection.

*2 Direct download from USB memory to a PC via a USB cable is not supported - please use a LAN connection and the FTP server.



FFT Analysis Function

MR8875 Ver. 2.01 or later

Simultaneously measure four phenomena

The MR8875's FFT analysis function can simultaneously analyze four phenomena with a single measurement.

By performing FFT analysis of different signal inputs from channels 1 through 4, it is possible to analyze the frequency components of each channel occurring at the same time.

Additionally, you can simultaneously view the linear spectrum, RMS spectrum, power spectrum, and phase spectrum for a signal input to channel 1, for example.

Analysis functionality for a variety of measurement scenarios

The MR8875 features calculation functions that are often used during field measurements. The linear spectrum is used in analysis that focuses on waveform amplitude values, while the power spectrum is used in analysis that focuses on energy, for example noise and vibration measurement. You can select the calculation function that best suits your application— for example, use a transfer function for measurement that identifies internal systems based on I/O characteristics.

Peak value display function (marker display)




The peak value display function can be used to search for maximum and local maximum values and then display them. Characteristic values can be easily displayed even without using a cursor. Since the MR8875 stores up to 200 frames (200 calculation results) of data, it will automatically search for the peak value again if a different frame is selected.

Running spectrum display function

The MR8875's running spectrum display function can be used to continuously display spectra that change over time. Up to 200 frames* of the most recent calculation results can be stored. Although Hioki's MR8847 Series only supports running spectrum display for certain types of calculations, the MR8875 can generate this display with all FFT calculation functions. Additionally, if the selected frame is changed, the cursor value can also be loaded.

* Frame data is stored in the instrument's internal memory, regardless of whether the running spectrum display is used.

The MR8875 can also freeze the spectrum display on its screen during measurement. This function allows data to be observed without the inclusion of unneeded information on the screen or in the data. All calculation results can be output as CSV data, which can be loaded into a spreadsheet application such as Microsoft Excel and used to create a three-dimensional graph.

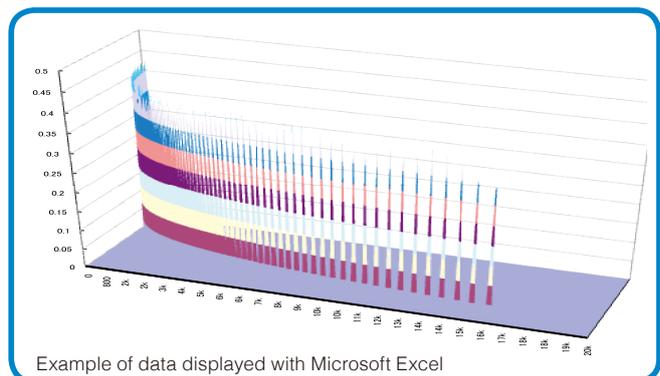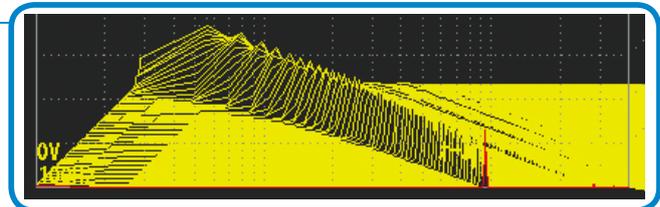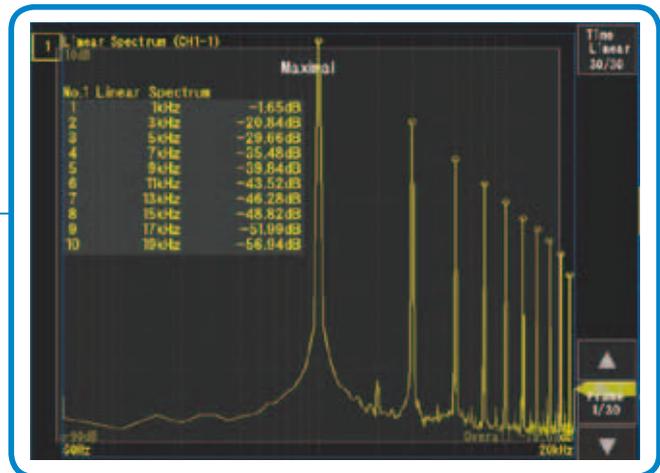

Extensive window functions

The MR8875 provides a total of seven window functions, including rectangular and Hanning variants. The rectangular function is used for analysis that focuses on spectrum amplitude values, while the Hanning function is used for analysis that focuses on the degree of spectral separation of frequency components. Additionally, by using an exponential window in impact measurement utilizing an impulse hammer, the instrument enables more precise analysis by limiting unneeded noise components on the time axis.

Continuous calculation function

When analyzing a signal that changes over time, the number of FFT calculation points becomes a limitation, preventing the waveform from being analyzed in all time domains. Furthermore, using too many FFT points prevents the desired results from being obtained because the spectrum is averaged. The MR8875 resolves these problems with its continuous calculation function. For data covering extended periods of time, calculation points can be shifted by a number of skip points* at a uniform interval. Moreover, calculations for up to 200 frames can be accomplished with a single operation. Calculation results for different time periods can be reviewed by changing the calculation frame, regardless of whether you're using the running spectrum display or a single-screen display.

* The number of skip points can be set from 100 to 10,000.


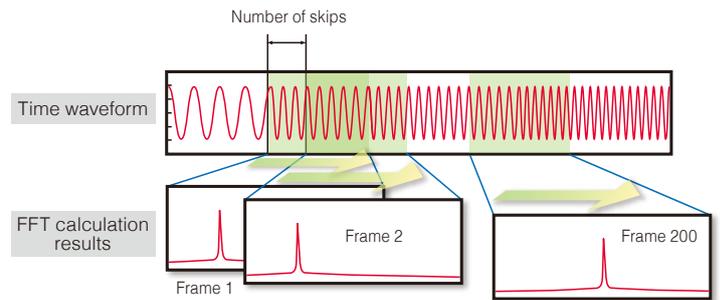


Illustration of continuous calculation


Overlay display function

The MR8875's overlay display function can be used to observe variations in waveforms captured using continuous measurement over time. Although previous Hioki models have not been able to overlay FFT calculations, the MR8875 offers this capability, improving the visibility of analysis.

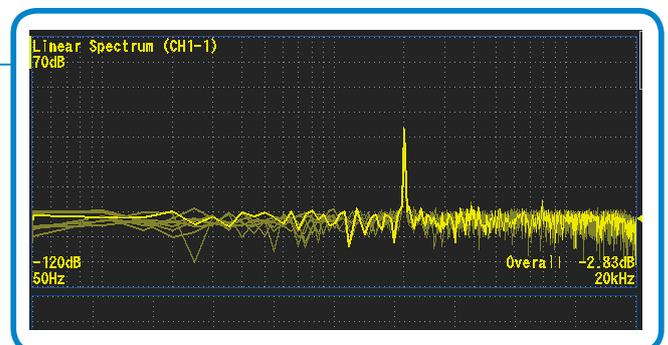

Visually appealing screen displays

The MR8875's display can be switched according to the application at hand. For example, its single-screen display can be used when focusing on the correlation between channels, while its four-screen display can be used to isolate complex spectra for viewing. Additionally, time and spectrum waveforms can be displayed above and below one another when focusing on correlation with a captured time waveform.

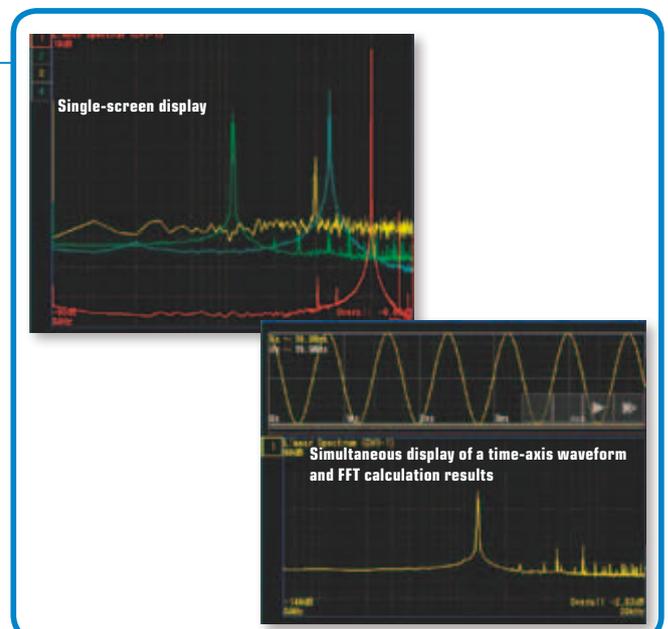


Waveform Calculation Function

MR8875 Ver. 2.01 or later

Real-time inter-channel calculation


The MR8875 features a new real-time inter-channel calculation* function that allows you to observe and record results for up to two calculations on the same input module while measurement continues.

* *Between channels on the same input module only (supported input modules: MR8901/8902/8903).*
 * *Calculations between different modes on the MR8902/8903 (voltage and temperature, etc.) are not supported.*

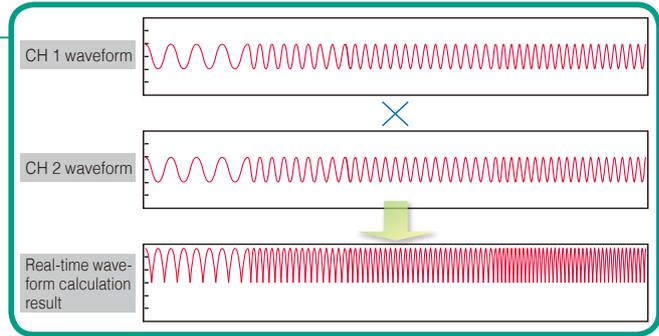

Waveform-dimension calculations

The previous MR8875 firmware version only supported calculations that generated values such as averages and RMS values, but the new version can process for up to eight calculations simultaneously, including the four arithmetic operations as well as differential-integral and other waveform-dimension calculations.

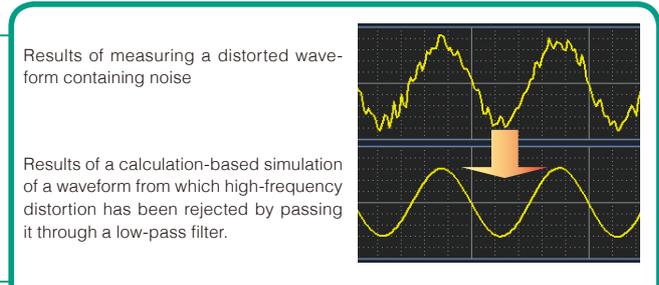


Digital filter calculations

The MR8875 offers new digital filter calculations* as part of its selection of waveform processing calculations, allowing the necessary bandwidth portion of a waveform containing noise to be calculated and the resulting waveform displayed.

* *Finite impulse response (FIR) and infinite impulse response (IIR) digital filters are offered. LPF (passing only the low-frequency component), HPF (passing only the high-frequency component), BPF, and BEF (passing or rejecting only a frequency bandwidth of a certain width) variants of each can be configured.*

* *Although FIR calculation processing is time-consuming, it can yield waveforms with no phase distortion. By contrast, IIR calculation yields results at a relatively faster calculation speed but is prone to phase distortion. Each filter's cutoff frequency is use-specified.*

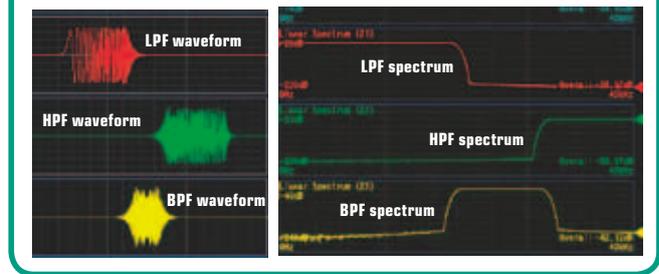

Principle FFT calculation functions

Calculation points	1,000	✓
	2,000	✓
	5,000	✓
	10,000	✓
	20,000	N/A
Window functions	Rectangular window	✓
	Hanning	✓
	Hamming	✓
	Blackman	✓
	Blackman-Harris	✓
	Flat top	✓
	Exponential	✓
Display	Amplitude	✓
	Real part	✓
	Imaginary part	✓
	Nyquist	N/A
	Peak value display	Local maximum Maximum
Averaging	Running spectrum (spectrogram)	✓ (200 lines)
	Phase highlighting	N/A
	Screen segmenting	1-/2-/4-screen waveform display
	Time (simple)	N/A
Averaging	Time (exponential)	✓
	Frequency (simple)	✓
	Frequency (exponential)	✓
	Frequency (peak hold)	✓

Principle FFT calculation functions

Analysis functions	Storage waveform	N/A
	Frequency distribution	N/A
	Linear spectrum	✓
	RMS spectrum	✓
	Power spectrum	✓
	Power spectrum density	N/A
	LPC analysis	N/A
	Transfer function	✓
	Cross power spectrum	✓
	Impulse response	N/A
	Coherence function	✓
	Phase spectrum	✓
	Auto-correlation function	N/A
Cross-correlation function	N/A	
Other	1/1-octave analysis	N/A
	1/3-octave analysis	N/A
	Frequency range	1.33 mHz to 400 kHz
	Max. number of simultaneous functions	✓
	Calculations targeting thinned data	N/A
	Recalculation after changing number of calculation points	N/A
	Total harmonic distortion (THD) analysis	✓
	Overall value	✓
	Anti-aliasing filter (AAF)	N/A
	Window function energy correction	✓
dB scaling	✓	
Continuous calculation	✓	
Calculation precision	32-bit floating point (IEEE single-precision)	

7 CAN Signal Input for Vehicle Testing

Synchronized mixed recording of CAN data and real data such as voltage, temperature, or distortion signals

CAN bus signals that are used widely, particularly in automotive applications, can be recorded, analyzed, converted to analog waveforms, and viewed. Simultaneous recording and viewing of analog waveforms from sensors, in addition to the CAN data, allows you to check the impact of noise and level changes on the communication data.



Vector's CAN database can be loaded using supplied software

Industry standard CANdb® database files can be loaded into the supplied setting software and associated to the CAN channel signals. CAN messages can be viewed using the customer-specified message and signal names, as well as scaled engineering units. Since parameters such as signal data type, start bit, length, and byte sequence are all pre-defined in CANdb, users can concentrate on their measurement tasks without needing to define signals.



CAN editor (bundled software)

Withstand extreme environmental temperatures, vibrations, and data loss due to power outages

In road tests, extreme environmental conditions associated with the temperature and vibration are harsh for measuring instruments. The **MR8875** has the wide operating temperature range of -10°C to 50°C and is compliant with the JIS D1601 standard for vibration resistance performance. It is designed to withstand the harsh conditions for in-vehicle measurement.

In the event of a power outage while data is being recorded, the power supply is maintained using a built-in large-capacity capacitor until data is completely written to the SD or USB memory. Risk of data loss or damage to the file system is minimized, and after power is restored, measurement can be restarted automatically.



Basic Specifications (Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year)	
Measurement function	High-speed recording
No. of input modules that can be installed	Up to 4 slots, user installable in any combination by plugging into the main unit [MR8901 ×4]: 16 analog channels + standard 8 logic and 2 pulse channels [MR8905 ×4]: 8 analog channels + standard 8 logic and 2 pulse channels [MR8902 ×4]: 60 analog channels + standard 8 logic and 2 pulse channels [MR8903 ×4]: 16 analog channels + standard 8 logic and 2 pulse channels [MR8904 ×4]: 8 CAN ports (analyzed 60 analog + analyzed 64 logic ch) + standard 8 logic and 2 pulse channels <i>* For analog units, channels are isolated from each other and from the MR8875's GND. For CAN unit ports or standard logic terminals or standard pulse terminals, all channels have common GND.</i>
Max. sampling rate	MR8901/MR8905: 500 kS/s (2 μs period, all channels simultaneously) MR8902: 10 msec (channel scanning) MR8903: 200 kS/s (5 μs period, all channels simultaneously) External sampling: 200 kS/s (5 μs period)
Storage memory capacity	Total 32 M-words (memory expansion: none, 8 MW/module) <i>* 1 word = 2 bytes, therefore 32 Mega-words = 64 Mega-bytes. * Memory can be allocated depending on the number of channels used at each input module</i>
External storage	SD card slot ×1, USB memory stick (USB 2.0 standard) <i>* FAT-16 or FAT-32 format on SD or USB</i>
Backup functions (At 23°C/ 73°F)	Clock and parameter setting backup: at least 10 years Waveform backup function: none
Interfaces	LAN ×1: 100BASE-TX (DHCP, DNS supported, FTP server/ client, Web server, send E-mail, command control) USB series mini-B receptacle × 1 (setting and measurement by communications commands, transfer data from SD card to a PC) USB series mini-A receptacle × 2 (USB memory stick, USB mouse, USB keyboard)
External control connectors	External trigger input, trigger output, external sampling input, pulse input ×2, external input ×3, external output ×2
External power supply	Three lines, +5V, 2A total output <i>* Connectable to three 9322 differential probes via power cord 9328</i>
Operating temperature and humidity (No condensation)	Temperature: -10°C to 40°C (14°F to 104°F), 80 % rh or less 40°C to 45°C (104°F to 113°F), 60 % rh or less 45°C to 50°C (113°F to 122°F), 50 % rh or less When powered by the battery pack: 0°C to 40°C (32°F to 104°F), 80 % rh or less When charging the battery pack: 10°C to 40°C (50°F to 104°F), 80 % rh or less Storage: -20°C to 40°C (-4°F to 104°F), 80 % rh or less 40°C to 45°C (104°F to 113°F), 60 % rh or less 45°C to 50°C (113°F to 122°F), 50 % rh or less Battery pack storage: -20°C to 40°C (-4°F to 104°F), 80 % rh or less
Applicable standards	Safety: EN61010-1, EMC: EN61326, EN61000-3-2, EN61000-3-3
Compliance standards	Anti-vibration: JIS D1601: 1995 5.3 (1) Corresponds to Class 1: a passenger car, Condition: class A
Power supply	AC adapter Z1002: 100 to 240 V AC (50/60 Hz) Battery Pack Z1003: 7.2 V DC Continuous operation times: one hour with back light ON (AC adapter has priority when used in combination with battery pack) DC power supply: 10 to 28 V DC (please contact your Hioki distributor for connection cord)
Charging function (At 23°C/ 73°F)	Recharging time: Approx. 3 hours (using the AC adapter and main unit to recharge the Battery Pack Z1003)
Power consumption	When using the AC adapter Z1002, or external DC power supply: 56 VA When using the battery pack: 36 VA
Dimensions and mass	Approx. 298W × 224H × 84D mm (11.73W × 8.82H × 3.31D in), 2.4 kg (84.7 oz), (excluding input modules and battery pack) Reference data: 2.75 kg (97.0 oz, excluding input modules and including battery pack), 3.47 kg (122.4 oz, including MR8901 ×4 and battery pack)
Supplied accessories	Instruction manual ×1, Measurement guide ×1, AC adapter Z1002 ×1, Protection sheet ×1, USB cable ×1, Shoulder strap ×1, Application disk (Wave viewer Wv, communication commands table, CAN Editor) ×1
Display	
Display type	8.4 inch SVGA-TFT color LCD (800 × 600 dots, with touch screen), (time axis 25 div × voltage axis 20 div, X-Y waveform 20 div × 20 div)
Screen settings	Waveform split screen (1, 2, or 4), X-Y 1 & X-Y 2 screens, time axis + X-Y waveform screen, sheet display (sheet all, sheet 1 to 4 selectable)
Screen display types	<ul style="list-style-type: none"> • Waveform display • Simultaneous waveform and gauge display • Simultaneous waveform, gauge, and settings display • Simultaneous waveform and numerical calculation results display • Waveform and A/B, C/D, E/F cursor values displayed at the same time • Simultaneous waveform and instantaneous value display
Waveform monitor	See waveform without recording (setting screen, waiting for trigger screen)
Real-time value monitor	Values for all channels can be monitored during measurement (Instantaneous value, average value, P-P value, Max. value, Min. value)
Display functions (Ver. 1.00 or later)	<ul style="list-style-type: none"> • Waveform scroll (scroll backwards through the display trend graph to view pas waveforms even while recording) • Event marker input and jump functions (up to 1000 markers) • Waveform inversion (positive/ negative) • Cursor readout (use A/B/C/D/E/F cursors) • Vernier display (fine amplitude adjustment)
Display functions (Ver. 2.01 or later)	<ul style="list-style-type: none"> • Waveform zoom (splits the screen vertically; supports waveform magnification and overall display) • Waveform overlay (select from off, overlay for each measurement, overlay at user-selected timing) • Waveform history (up to 16 past data sets can be selected and displayed.)

Measurement function (High-speed recording)	
Time axis	200 μs, 500 μs/div, 1 ms to 500 ms/div, 1 s to 5 min/div, 21 ranges, external sampling (max. 200 kS/s), Recording interval time at real-time save ON: 2 μs/S (channels up to 2), 5 μs/S (channels up to 8), 10 μs/S (channels up to 16), 20 μs/S (channels up to 30), 50 μs/S (channels up to 64), 100 μs/S (with no limit on number of channels in use)
Accuracy of time axis	± 0.0005 %
Time axis resolution	100 points /div
Recording length (with MR8901 × 4, logic and pulse inputs OFF)	25 to 20,000 div *1 *2, 50,000 div *3, or user-configurable from 5 to 80,000 div *3 in 1 div increments *1: 4 ch/module, *2: 2 ch/module, *3: 1 ch/module
Waveform expansion, compression	Time axis: ×10 to ×2 or ×1, ×1/2 to ×1/50,000 Voltage axis: ×100 to ×2, ×1, ×1/2 to ×1/10 Upper and lower limit settings, or position setting
Pre-trigger	(Trigger timing: At start) Pre-trigger data can be recorded for an interval set in steps ranging from 0 to 100 % of the recording length.
Post-trigger	(Trigger timing: At stop) Post-trigger data can be recorded for an interval set in steps ranging from 0 to 40 % of the recording length
Real-time data save	ON /OFF selectable (exclusive real-time save or automatic save) Function: Waveforms are saved as binary data to the SD memory card at each interval (Note: Cannot save in real-time to a USB memory, use only SD memory cards sold by Hioki) Endless loop saving: New file overwrites the oldest file when the SD memory card capacity runs short (Note: Delete files only at saved repeat trigger mode) Normal saving: Saving stops when the SD memory card capacity is full
Auto data save	Select from Off, waveform data (Binary or CSV), numerical calculation results, and image data (compressed BMP or PNG). Function: Data are saved to either SD memory card or USB memory stick at once after the specified recording length is acquired. Endless loop saving: New file overwrites the oldest file when the SD memory card or USB memory capacity runs short Normal saving: Saving stops when the SD memory card or USB memory capacity is full
Data protection	In the event of a power outage during saving to storage media, the file is closed and then the power is shut down. Note: This function is enabled 15 minutes after the power is turned on.
Loading data from media	<ul style="list-style-type: none"> • Binary data stored in the SD memory card or the USB memory stick can be recalled by the MR8875 internal storage memory • Waveform data saved in real time to the SD memory card can be loaded starting at a specified position up to the maximum storage memory capacity.
Memory segmentation	N/A
Trigger functions	
Mode	Single, Repeat
Timing	Start / Stop / Start & Stop (separate trigger conditions can be set to start and stop)
Trigger sources	<ul style="list-style-type: none"> • Trigger source selectable for each channel (Free-running when all trigger sources are off) • Analog input: Select up to 4 channels for each module • Inter-channel calculation results: W1-1 to W4-2 (Ver.2.01 or later) • Logic input: LA1 to LA4, LB1 to LB2 (4 channels × 2 probes), CAN L1 to L6 (for each MR8904 CAN Unit). Pattern triggers can be configured for each of the above trigger sources. • Pulse input: P1, P2 (2 channels) • External input: Input signal to external trigger terminal • Logical AND/ OR of all sources • Forced trigger execution: Priority over any other trigger source • Interval trigger: Trigger is activated at recording start, and again at each set interval
Trigger types (Analog, pulse)	<ul style="list-style-type: none"> • Level: A trigger is applied when rise or fall to set voltage value. • Window: Set the upper and lower limits of trigger level
Trigger types (Logic)	<ul style="list-style-type: none"> • Logic pattern: Settable to 1, 0, or × for each logic probes • The trigger condition (AND/OR) can be set between logic input channels in each probe.
Trigger types (External input)	<ul style="list-style-type: none"> • Rise or fall selectable (max. allowable input voltage 10 V DC) Rising: A trigger is applied when rise from "Low" (0 to 0.8 V) to "High" (2.5 to 10 V) Falling: A trigger is applied when fall from "High" (2.5 to 10 V) to "Low" (0 to 0.8 V) or terminal short. • External trigger filter and response pulse width: When external filter Off: H period 1 ms or greater, L period 2 μs or greater When external filter On: H period 2.5 ms or greater, L period 2.5 ms or greater
Trigger level resolution	<ul style="list-style-type: none"> • Analog: 0.1 % f.s. (f.s.=20 div) Note: With the CAN Unit MR8904, resolution fluctuates according to the bit length defined by the CAN • Pulse integration: 0.002 % f.s., • Pulse rotation count: 0.02 % f.s. (f.s.=20 div)
Trigger filter	Set by number of samples (Off, 10 to 1000 points)
Trigger output	<ul style="list-style-type: none"> • Open drain output (with 5 voltage output, active Low) • Output voltage: 4.0 to 5.0 V (high level), 0 to 0.5 V (low level) • Output pulse width: Selectable level or pulse Level: Sampling period × (number of data since trigger -1) or longer (2 μs or longer) Pulse: 2 ms ±10%

Calculation functions	
Real-time inter-channel calculations (Ver.2.01 or later)	<ul style="list-style-type: none"> Up to 2 calculations per module can be performed simultaneously. Calculation target: Analog Unit MR8901, Voltage/Temp Unit MR8902, Strain Unit MR8903 <i>Inter-channel calculations are limited to single module.</i> <i>Scaling and probe settings for calculation channels targeted for calculations are disabled.</i> <i>Calculation results can be scaled.</i> <i>Calculations between different modes on the MR8902 and MR8903 are not supported.</i> Calculations: Addition, subtraction, multiplication
Numerical calculation	<ul style="list-style-type: none"> Up to 8 calculations can be performed simultaneously Calculation target: Internal memory Calculations: Average, effective (rms), peak to peak, maximum value, time to maximum value, minimum value, time to minimum value, period, frequency, rise time, fall time, area value, X-Y area value, standard deviation, specified level time, specified time level, pulse width, duty ratio, pulse count, time difference, phase difference, high-level, low-level, four arithmetic operations, Calculation results can be saved to SD memory card or USB memory stick. Calculation range: Select from all measurement data or between A/B or C/D cursors Automatic storing of calculation results in CSV format to the SD card or the USB memory stick.
Waveform calculations (Ver.2.01 or later)	<ul style="list-style-type: none"> Up to 8 calculations can be performed simultaneously. Calculation target: Internal memory Calculations: Basic arithmetic, absolute value, exponents, common logarithms, square roots, differentials (1st and 2nd order), integrals (1st and 2nd order), moving averages, time-axis moving averages, trigonometric operations (SIN, COS, TAN), inverse trigonometric operations (ASIN, ACOS, ATAN), FIR filter operations, IIR filter operations, average value, maximum value, minimum value, level at time Calculation range: All measurement data; areas between the A/B and C/D cursors can be selected.
FFT calculations (Ver.2.01 or later)	<ul style="list-style-type: none"> Up to 4 calculations can be performed simultaneously. Calculation target: Internal memory Calculation modes: Single, repeat Number of points: 1000 to 10000 Number of skips: Automatic, 100 to 10000 <i>Can be set only when the calculation mode is "Repeat".</i> Window functions: Rectangular window, Hanning, Hamming, Blackman, Blackman-Harris, flat top, exponential Averaging: Off, simple average, indexed average, peak hold Compensation: None, power, average Peak value display: Off, local maximum value, maximum value Analysis mode: Off, linear spectrum, RMS spectrum, power spectrum, transmission function, cross-power spectrum, coherence function, phase spectrum Display scale: Linear scale, log scale
Evaluation	Calculation result evaluation output: GO/NG (with open-drain 5 V output)

Other functions	
External sampling	Maximum input: Up to 10 V DC Maximum input frequency: 200 kHz Input signal condition: High level 2.5 to 10 V, Low level 0 to 0.8 V, Pulse width H or L 2.5 μ s or longer
Other	<ul style="list-style-type: none"> Scaling, Comment entry, Select from time, date, and number of data for the horizontal axis display, Key lock Beep sound ON/OFF Auto range setting (automatically sets the best suitable sampling rate and amplitude range) Hold start condition (when the power is interrupted during recording, measurement automatically resumes after power is restored) Auto set up (automatically load setting files stored in internal memory or the SD card) Save the setting condition in internal memory (up to 6 conditions) Manual data save


Pulse input section		
No. of channels	2 channels, push button type terminal, not isolated (common GND with main unit)	
Mode	Rotation, Integration	
Measurement functions	<ul style="list-style-type: none"> Divided rotation: 1 to 50,000 count (Rotation number: number of pulses per rotation; Integration: number of pulses per count) Timing: Select from "starting the count at the trigger" or "at the start of measurement" Integration mode: Select from "integration from the start of measurement" or "instantaneous value at each sampling period" Processing of integration overflows: Select either "value returns to 0 and counting continues" or "the overflow state persists" 	
Input form	<ul style="list-style-type: none"> No-voltage 'a' contact (normally open contact), No-voltage 'b' contact (normally short contact), Open collector or voltage input Input resistance: 1.1 MΩ 	
Max. allowable input	0 V to 50 V DC (max. voltage between input terminals that does not cause damage)	
Max. rated voltage between channels	Not isolated (common GND with main unit)	
Max. rated voltage to earth	Not isolated (common GND with main unit)	
Detect level	4 V: (High: over 4.0 V, Low: 0 to 1.5 V) 1 V: (High: over 1.0 V, Low: 0 to 0.5 V)	
Pulse input period	With filter Off: 200 μ s or more (both H and L periods must be at least 100 μ s) With filter On: 100 ms or more (both H and L periods must be at least 50 ms)	
Slope	Count at rising edge, or count at falling edge	
Filter	Chatter prevention filter (On/Off switchable)	
Setting range	Resolution	Measurement range
2,500 c/div	1 c/LSB	0 to 65,535 c
25k c/div	10 c/LSB	0 to 655,350 c
250k c/div	100 c/LSB	0 to 6,553,500 c
5M c/div	2k c/LSB	0 to 131,070,000 c
125M c/div	50k c/LSB	0 to 3,276,750,000 c
Rotation: 250 [r/s]/div	1 [r/s]/LSB	0 to 5,000 [r/s]

Maximum time to record to the internal storage memory


* The maximum number of channels to be used is 16 because memory for recording to the internal memory is allocated to each input module.
 * Built-in logic, and pulses P1 and P2 each use the capacity equivalent to one analog channel.

Number of channels to be used * Number of channels for input module with most enabled-measurement channels	9 to 16 ch						5 to 8 ch					3 to 4 ch				2 ch			1 ch					
	Time axis	Sampling	5000 div	10,000 div	20,000 div	40,000 div	80,000 div	5000 div	10,000 div	20,000 div	40,000 div	80,000 div	5000 div	10,000 div	20,000 div	40,000 div	80,000 div	5000 div	10,000 div	20,000 div				
200 μ s/div	2 μ s	1 s	2 s	4 s	8 s	16 s	200 μ s/div	2 μ s	1 s	2 s	4 s	8 s	200 μ s/div	2 μ s	1 s	2 s	4 s	200 μ s/div	2 μ s	1 s	2 s	4 s	8 s	16 s
500 μ s/div	5 μ s	2.5 s	5 s	10 s	20 s	40 s	500 μ s/div	5 μ s	2.5 s	5 s	10 s	20 s	500 μ s/div	5 μ s	2.5 s	5 s	10 s	500 μ s/div	5 μ s	2.5 s	5 s	10 s	20 s	40 s
1 ms/div	10 μ s	5 s	10 s	20 s	40 s	1 min 20 s	1 ms/div	10 μ s	5 s	10 s	20 s	40 s	1 ms/div	10 μ s	5 s	10 s	20 s	1 ms/div	10 μ s	5 s	10 s	20 s	40 s	1 min 20 s
2 ms/div	20 μ s	10 s	20 s	40 s	1 min 20 s	2 min 40 s	2 ms/div	20 μ s	10 s	20 s	40 s	1 min 20 s	2 ms/div	20 μ s	10 s	20 s	40 s	2 ms/div	20 μ s	10 s	20 s	40 s	1 min 20 s	2 min 40 s
5 ms/div	50 μ s	25 s	50 s	1 min 40 s	3 min 20 s	6 min 40 s	5 ms/div	50 μ s	25 s	50 s	1 min 40 s	3 min 20 s	5 ms/div	50 μ s	25 s	50 s	1 min 40 s	5 ms/div	50 μ s	25 s	50 s	1 min 40 s	3 min 20 s	6 min 40 s
10 ms/div	100 μ s	50 s	1 min 40 s	3 min 20 s	6 min 40 s	13 min 20 s	10 ms/div	100 μ s	50 s	1 min 40 s	3 min 20 s	6 min 40 s	10 ms/div	100 μ s	50 s	1 min 40 s	3 min 20 s	10 ms/div	100 μ s	50 s	1 min 40 s	3 min 20 s	6 min 40 s	13 min 20 s
20 ms/div	200 μ s	1 min 40 s	3 min 20 s	6 min 40 s	13 min 20 s	26 min 40 s	20 ms/div	200 μ s	1 min 40 s	3 min 20 s	6 min 40 s	13 min 20 s	20 ms/div	200 μ s	1 min 40 s	3 min 20 s	6 min 40 s	20 ms/div	200 μ s	1 min 40 s	3 min 20 s	6 min 40 s	13 min 20 s	26 min 40 s
50 ms/div	500 μ s	4 min 10 s	8 min 20 s	16 min 40 s	33 min 20 s	1 h 06 min 40 s	50 ms/div	500 μ s	4 min 10 s	8 min 20 s	16 min 40 s	33 min 20 s	50 ms/div	500 μ s	4 min 10 s	8 min 20 s	16 min 40 s	50 ms/div	500 μ s	4 min 10 s	8 min 20 s	16 min 40 s	33 min 20 s	1 h 06 min 40 s
100 ms/div	1 ms	8 min 20 s	16 min 40 s	33 min 20 s	1 h 06 min 40 s	2 h 13 min 20 s	100 ms/div	1 ms	8 min 20 s	16 min 40 s	33 min 20 s	1 h 06 min 40 s	100 ms/div	1 ms	8 min 20 s	16 min 40 s	33 min 20 s	100 ms/div	1 ms	8 min 20 s	16 min 40 s	33 min 20 s	1 h 06 min 40 s	2 h 13 min 20 s
200 ms/div	2 ms	16 min 40 s	33 min 20 s	1 h 06 min 40 s	2 h 13 min 20 s	4 h 26 min 40 s	200 ms/div	2 ms	16 min 40 s	33 min 20 s	1 h 06 min 40 s	2 h 13 min 20 s	200 ms/div	2 ms	16 min 40 s	33 min 20 s	1 h 06 min 40 s	200 ms/div	2 ms	16 min 40 s	33 min 20 s	1 h 06 min 40 s	2 h 13 min 20 s	4 h 26 min 40 s
500 ms/div	5 ms	41 min 40 s	1 h 23 min 20 s	2 h 46 min 40 s	5 h 33 min 20 s	11 h 06 min 40 s	500 ms/div	5 ms	41 min 40 s	1 h 23 min 20 s	2 h 46 min 40 s	5 h 33 min 20 s	500 ms/div	5 ms	41 min 40 s	1 h 23 min 20 s	2 h 46 min 40 s	500 ms/div	5 ms	41 min 40 s	1 h 23 min 20 s	2 h 46 min 40 s	5 h 33 min 20 s	11 h 06 min 40 s
1 s/div	10 ms	1 h 23 min 20 s	2 h 46 min 40 s	5 h 33 min 20 s	11 h 06 min 40 s	22 h 13 min 20 s	1 s/div	10 ms	1 h 23 min 20 s	2 h 46 min 40 s	5 h 33 min 20 s	11 h 06 min 40 s	1 s/div	10 ms	1 h 23 min 20 s	2 h 46 min 40 s	5 h 33 min 20 s	1 s/div	10 ms	1 h 23 min 20 s	2 h 46 min 40 s	5 h 33 min 20 s	11 h 06 min 40 s	22 h 13 min 20 s
2 s/div	20 ms	2 h 46 min 40 s	5 h 33 min 20 s	11 h 06 min 40 s	22 h 13 min 20 s	1 d 20 h 26 min 40 s	2 s/div	20 ms	2 h 46 min 40 s	5 h 33 min 20 s	11 h 06 min 40 s	22 h 13 min 20 s	2 s/div	20 ms	2 h 46 min 40 s	5 h 33 min 20 s	11 h 06 min 40 s	2 s/div	20 ms	2 h 46 min 40 s	5 h 33 min 20 s	11 h 06 min 40 s	22 h 13 min 20 s	1 d 20 h 26 min 40 s
5 s/div	50 ms	6 h 56 min 40 s	13 h 53 min 20 s	1 d 03 h 46 min 40 s	2 d 07 h 33 min 20 s	4 d 15 h 06 min 40 s	5 s/div	50 ms	6 h 56 min 40 s	13 h 53 min 20 s	1 d 03 h 46 min 40 s	2 d 07 h 33 min 20 s	5 s/div	50 ms	6 h 56 min 40 s	13 h 53 min 20 s	1 d 03 h 46 min 40 s	5 s/div	50 ms	6 h 56 min 40 s	13 h 53 min 20 s	1 d 03 h 46 min 40 s	2 d 07 h 33 min 20 s	4 d 15 h 06 min 40 s
10 s/div	100 ms	13 h 53 min 20 s	1 d 03 h 46 min 40 s	2 d 07 h 33 min 20 s	4 d 15 h 06 min 40 s	9 d 06 h 13 min 20 s	10 s/div	100 ms	13 h 53 min 20 s	1 d 03 h 46 min 40 s	2 d 07 h 33 min 20 s	4 d 15 h 06 min 40 s	10 s/div	100 ms	13 h 53 min 20 s	1 d 03 h 46 min 40 s	2 d 07 h 33 min 20 s	10 s/div	100 ms	13 h 53 min 20 s	1 d 03 h 46 min 40 s	2 d 07 h 33 min 20 s	4 d 15 h 06 min 40 s	9 d 06 h 13 min 20 s
30 s/div	300 ms	1 d 17 h 40 min	3 d 11 h 20 min	6 d 22 h 40 min	13 d 21 h 20 min	27 d 18 h 40 min	30 s/div	300 ms	1 d 17 h 40 min	3 d 11 h 20 min	6 d 22 h 40 min	13 d 21 h 20 min	30 s/div	300 ms	1 d 17 h 40 min	3 d 11 h 20 min	6 d 22 h 40 min	30 s/div	300 ms	1 d 17 h 40 min	3 d 11 h 20 min	6 d 22 h 40 min	13 d 21 h 20 min	27 d 18 h 40 min
50 s/div	500 ms	2 d 21 h 26 min 40 s	5 d 18 h 53 min 20 s	11 d 13 h 46 min 40 s	23 d 03 h 33 min 20 s	46 d 07 h 06 min 40 s	50 s/div	500 ms	2 d 21 h 26 min 40 s	5 d 18 h 53 min 20 s	11 d 13 h 46 min 40 s	23 d 03 h 33 min 20 s	50 s/div	500 ms	2 d 21 h 26 min 40 s	5 d 18 h 53 min 20 s	11 d 13 h 46 min 40 s	50 s/div	500 ms	2 d 21 h 26 min 40 s	5 d 18 h 53 min 20 s	11 d 13 h 46 min 40 s	23 d 03 h 33 min 20 s	46 d 07 h 06 min 40 s
60 s/div	600 ms	3 d 11 h 20 min	6 d 22 h 40 min	13 d 21 h 20 min	27 d 18 h 40 min	55 d 13 h 20 min	60 s/div	600 ms	3 d 11 h 20 min	6 d 22 h 40 min	13 d 21 h 20 min	27 d 18 h 40 min	60 s/div	600 ms	3 d 11 h 20 min	6 d 22 h 40 min	13 d 21 h 20 min	60 s/div	600 ms	3 d 11 h 20 min	6 d 22 h 40 min	13 d 21 h 20 min	27 d 18 h 40 min	55 d 13 h 20 min
100 s/div	1.0 s	5 d 18 h 53 min 20 s	11 d 13 h 46 min 40 s	23 d 03 h 33 min 20 s	46 d 07 h 06 min 40 s	92 d 14 h 13 min 20 s	100 s/div	1.0 s	5 d 18 h 53 min 20 s	11 d 13 h 46 min 40 s	23 d 03 h 33 min 20 s	46 d 07 h 06 min 40 s	100 s/div	1.0 s	5 d 18 h 53 min 20 s	11 d 13 h 46 min 40 s	23 d 03 h 33 min 20 s	100 s/div	1.0 s	5 d 18 h 53 min 20 s	11 d 13 h 46 min 40 s	23 d 03 h 33 min 20 s	46 d 07 h 06 min 40 s	92 d 14 h 13 min 20 s
2 min/div	1.2 s	6 d 22 h 40 min	13 d 21 h 20 min	27 d 18 h 40 min	55 d 13 h 20 min	111 d 02 h 40 min	2 min/div	1.2 s	6 d 22 h 40 min	13 d 21 h 20 min	27 d 18 h 40 min	55 d 13 h 20 min	2 min/div	1.2 s	6 d 22 h 40 min	13 d 21 h 20 min	27 d 18 h 40 min	2 min/div	1.2 s	6 d 22 h 40 min	13 d 21 h 20 min	27 d 18 h 40 min	55 d 13 h 20 min	111 d 02 h 40 min
5 min/div	3.0 s	17 d 08 h 40 min	34 d 17 h 20 min	69 d 10 h 40 min	138 d 21 h 20 min	277 d 18 h 40 min	5 min/div	3.0 s	17 d 08 h 40 min	34 d 17 h 20 min	69 d 10 h 40 min	138 d 21 h 20 min	5 min/div	3.0 s	17 d 08 h 40 min	34 d 17 h 20 min	69 d 10 h 40 min	5 min/div	3.0 s	17 d 08 h 40 min	34 d 17 h 20 min	69 d 10 h 40 min	138 d 21 h 20 min	277 d 18 h 40 min

External appearance and dimensions

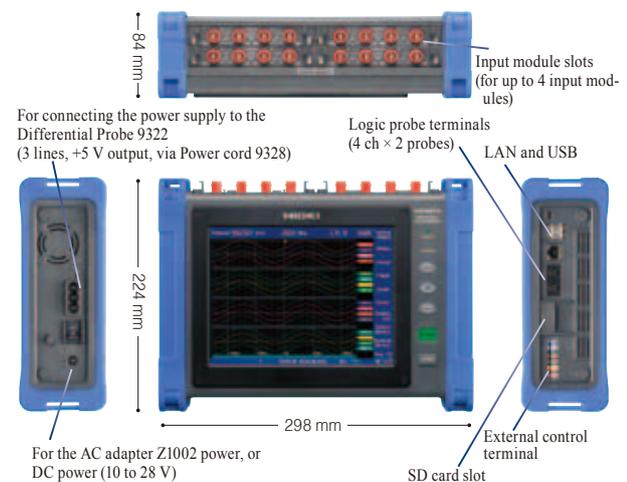

Options specifications (sold separately)



Plug-in slot for the input modules



Measurement target	Input module	Measurement range	Resolution
Voltage	Analog Unit MR8901	100 mV f.s. to 200 V f.s.	4 μ V
	Analog Unit MR8905	10 V f.s. to 1000 V f.s.	400 μ V
	Voltage/Temp Unit MR8902	10 mV f.s. to 100 V f.s.	0.5 μ V
	Strain Unit MR8903	1 mV f.s. to 20 mV f.s.	0.04 μ V
Current	Analog Unit MR8901 + optional current sensor	Depends on current sensor(s) in use * Certain current sensors require a separate power supply	1/1250 div
RMS AC voltage	Analog Unit MR8905 Analog Unit MR8901 + optional Differential Probe 9322	10 V rms f.s. to 700 V rms f.s. 100 V rms to 1 kV rms	400 μ V 1/1250 div
Temperature (Thermocouple)	Voltage/Temp Unit MR8902	200 $^{\circ}$ C f.s. to 2000 $^{\circ}$ C f.s. * Upper and lower limit values depend on the thermocouple in use	0.01 $^{\circ}$ C
Distortion, Stress	Strain Unit MR8903	400 μ e to 20,000 μ e f.s.	0.016 μ e
Analyze CAN signals	CAN Unit MR8904	2 ports /unit *Up to 13 analog channels each equivalent to a 16-bit analog signal *Up to 16 logic channels each equivalent to a 1-bit logic signal	N/A
Relay contacts, voltage on/off	Logic Probe 9320-01	Depends on logic probes in use * Max. input 50 V, threshold +1.4/+2.5/+4.0 V * Contact short/open, non voltage	N/A
AC/DC voltage on/off	Logic Probe MR9321-01	Depends on logic probes in use * Up to 250V AC/DC, detect live or not live	N/A

Dimensions, mass: Approx. 119.5W × 18.8H × 151.5D mm (4.70W × 0.74H × 5.96D in), Approx. 180 g (6.3 oz) Accessories: None



Analog Unit MR8901 (Accuracy at 23±5 $^{\circ}$ C/73±9 $^{\circ}$ F, 20 to 80% rh after 30 min. of warm-up time and zero adjustment, Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year)

Functions	No. of channels: 4, for voltage measurement
Input connectors	Isolated BNC connector (input resistance 1 M Ω , input capacitance 10 pF) Max. rated voltage to earth: 100 V AC, DC (with input isolated from the main unit, the max. voltage that can be applied between input channel and chassis and between input channels without damage)
Measurement range	5 mV to 10 V/div, 11 ranges, full scale: 20 div * AC voltage can be measured/displayed: up to 140 V rms at $\times 1/2$ amplitude compression, but limited to 100 V rms according as max. rated voltage to earth
Low-pass filter	Low-pass filter: 5/50/500 Hz, 5 kHz, OFF
Resolution	1/1250 of measurement range (using 16-bit A/D converter)
Highest sampling rate	500 kS/s (simultaneous sampling across 4 channels)
Accuracy	± 0.5 % of full scale (with filter 5 Hz, Zero position accuracy included)
Frequency characteristics	DC to 100 kHz -3 dB
Input coupling	DC/GND
Max. allowable input	150 V DC (the max. voltage that can be applied across input pins without damage)

Dimensions, mass: Approx. 119.5W × 18.8H × 184.8D mm (4.70W × 0.74H × 7.28D in), Approx. 190 g (6.7 oz) Accessories: Ferrite clamp $\times 2$



Voltage/Temp Unit MR8902 (Accuracy at 23±5 $^{\circ}$ C/73±9 $^{\circ}$ F, 20 to 80% rh after 30 minutes of warm-up time and zero adjustment, Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year)

Functions	No. of channels: 15, for voltage/temperature measurement (selectable for each channels)
Input connectors	Voltage/thermocouple input: push button terminal Recommended wire diameter: single-wire ϕ 0.32 mm to ϕ 0.65 mm, stranded wire 0.08 to 0.32 mm ² (conductor wire diameter min. ϕ 0.12 mm), AWG 28 to 22 Input resistance: 1 M Ω Max. rated voltage to earth: 100 V AC, DC (with input isolated from the main unit, the max. voltage that can be applied between input channel and chassis and between input channels without damage)
Voltage measurement ranges	500 μ V to 5 V/div, 9 ranges, full scale: 20 division * The AC instantaneous voltage waveform cannot be measured due to the slow sampling speed. Resolution: 1/1000 of measurement range (using 16-bit A/D converter) Accuracy: ± 0.1 % f.s. (with digital filter ON, Zero position accuracy included)
Temperature measurement range	Reference junction compensation: Internal/ External (selectable) Thermocouple broken-wire detection: ON/OFF (selection applies to entire unit) Thermocouple type: K, J, E, T, N, R, S, B, WRc5-26 * For thermocouple measurement ranges, resolution, and accuracy, refer to the specifications table below
Digital filter	50 Hz, 60 Hz, or OFF
Data refresh rate	10 ms (with filter OFF, burn-out detection OFF) 20 ms (with filter OFF, burn-out detection ON) 500 ms (with filter ON, data refresh rate: Fast) 2 s (with filter ON, data refresh rate: Normal)
Max. allowable input	100 V DC (the max. voltage that can be applied across input pins without damage)

MR8902 specifications

Thermocouples	Setting ranges (full scale=20 div)	Resolution	Measurement ranges	Accuracy
K	10 $^{\circ}$ C/div	0.01 $^{\circ}$ C	-100 to less than 0 $^{\circ}$ C 0 to 200 $^{\circ}$ C	± 0.8 $^{\circ}$ C ± 0.6 $^{\circ}$ C
			-200 to less than -100 $^{\circ}$ C -100 to 1000 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
	50 $^{\circ}$ C	0.05 $^{\circ}$ C	-200 to less than -100 $^{\circ}$ C -100 to 1000 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
			-200 to less than -100 $^{\circ}$ C -100 to 1350 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
	100 $^{\circ}$ C	0.1 $^{\circ}$ C	-200 to less than -100 $^{\circ}$ C -100 to less than 0 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
			-100 to less than 0 $^{\circ}$ C 0 to 200 $^{\circ}$ C	± 0.8 $^{\circ}$ C ± 0.6 $^{\circ}$ C
J	10 $^{\circ}$ C/div	0.01 $^{\circ}$ C	-100 to less than 0 $^{\circ}$ C 0 to 200 $^{\circ}$ C	± 0.8 $^{\circ}$ C ± 0.6 $^{\circ}$ C
			-200 to less than -100 $^{\circ}$ C -100 to 1000 $^{\circ}$ C	± 1.0 $^{\circ}$ C ± 0.8 $^{\circ}$ C
	50 $^{\circ}$ C	0.05 $^{\circ}$ C	-200 to less than -100 $^{\circ}$ C -100 to 1000 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
			-200 to less than -100 $^{\circ}$ C -100 to 1200 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
	100 $^{\circ}$ C	0.1 $^{\circ}$ C	-100 to less than -100 $^{\circ}$ C -100 to less than 0 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
			-100 to less than 0 $^{\circ}$ C 0 to 1000 $^{\circ}$ C	± 0.8 $^{\circ}$ C ± 0.6 $^{\circ}$ C
E	10 $^{\circ}$ C/div	0.01 $^{\circ}$ C	-100 to less than 0 $^{\circ}$ C 0 to 200 $^{\circ}$ C	± 0.8 $^{\circ}$ C ± 0.6 $^{\circ}$ C
			-200 to less than -100 $^{\circ}$ C -100 to less than 0 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
	50 $^{\circ}$ C	0.05 $^{\circ}$ C	-200 to less than -100 $^{\circ}$ C -100 to less than 0 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
			-200 to less than -100 $^{\circ}$ C -100 to less than 0 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
	100 $^{\circ}$ C	0.1 $^{\circ}$ C	-200 to less than -100 $^{\circ}$ C -100 to less than 0 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
			-100 to less than 0 $^{\circ}$ C 0 to 1000 $^{\circ}$ C	± 0.8 $^{\circ}$ C ± 0.6 $^{\circ}$ C
T	10 $^{\circ}$ C/div	0.01 $^{\circ}$ C	-100 to less than 0 $^{\circ}$ C 0 to 200 $^{\circ}$ C	± 0.8 $^{\circ}$ C ± 0.6 $^{\circ}$ C
			-200 to less than -100 $^{\circ}$ C -100 to less than 0 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
	50 $^{\circ}$ C	0.05 $^{\circ}$ C	-200 to less than -100 $^{\circ}$ C -100 to less than 0 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
			-200 to less than -100 $^{\circ}$ C 0 to 400 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.6 $^{\circ}$ C
	100 $^{\circ}$ C	0.1 $^{\circ}$ C	-200 to less than -100 $^{\circ}$ C -100 to less than 0 $^{\circ}$ C	± 1.5 $^{\circ}$ C ± 0.8 $^{\circ}$ C
			-100 to less than 0 $^{\circ}$ C 0 to 400 $^{\circ}$ C	± 0.8 $^{\circ}$ C ± 0.6 $^{\circ}$ C

Note: The thermocouple accuracy is obtained by adding a reference junction compensation accuracy of ± 0.5 $^{\circ}$ C



Dimensions, mass: Approx. 119.5W × 18.8H × 151.5D mm (4.70W × 0.74H × 5.96D in), Approx. 173 g (6.1 oz) Accessories: Conversion cable $\times 2$ (Connector: TAJIMI PRC03-12A10-7M10.5)



Strain Unit MR8903 (Accuracy at 23±5 $^{\circ}$ C/73±9 $^{\circ}$ F, 20 to 80% rh after 30 minutes of warm-up time and auto-balance, Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year)

Functions	No. of channels: 4, for voltage/strain measurements (selectable for each channel, electronic auto-balancing, balance adjustment range within ± 10000 μ V, ± 100000 μ e)
Input connectors	Unit side: "HDR-EC14LFDTG2-SLE+" made by Honda Tsushin Kogyo Co., Ltd. Japan Via conversion cable, "PRC03-12A10-7M10.5" made by Tajimi Electronics Co., Ltd. Japan Max. rated voltage to earth: 33 V ACrms or 70 V DC (with input isolated from the main unit, the max. voltage that can be applied between input channel and chassis and between input channels without damage)
Suitable transducer	Strain gauge converter, Bridge resistance: 120 Ω to 1 k Ω , Bridge voltage: 2 V ± 0.05 V, Gauge rate: 2.0
Input resistance	More than 1 M Ω
Voltage measurement ranges	50 μ V to 1000 μ V/div, 5 ranges, full scale: 20 division Accuracy: ± 0.5 % f.s. + 4 μ V (at 50 μ V/div only), other ranges ± 0.5 % f.s. (after auto-balance, with filter 5 Hz, zero position accuracy included)
Strain measurement ranges	20 μ e to 1000 μ e/div, 6 ranges, full scale: 20 division Accuracy: ± 0.5 % f.s. + 4 μ e (at 20, 50 μ e/div), other ranges ± 0.5 % f.s. (after auto-balance, with filter 5 Hz, zero position accuracy included)
Low-pass filter	Low-pass filter: 5/10/100 Hz, 1 kHz, OFF
Resolution	1/1250 of measurement range (using 16-bit A/D converter)
Highest sampling rate	200 kS/s (simultaneous sampling across 4 channels)
Frequency characteristics	DC to 20 kHz +1/-3 dB
Max. allowable input	10 V DC (the max. voltage that can be applied across input pins without damage)

Dimensions, mass: Approx. 119.5W × 18.8H × 151.5D mm (4.70W × 0.74H × 5.96D in), Approx. 185 g (6.5 oz) Accessories: None



CAN Unit MR8904

Input CAN port	Number of ports: 2, Connector: D-sub a male 9 pin $\times 2$
Standards	ISO 11898 CAN 2.0b, ISO 11898-1, ISO 11898-2, ISO 11898-3, SAE J2411
Interface	Selectable: High-speed CAN, Low-speed CAN, or Single-wire CAN by port (with built-in corresponding transceiver)
Transmit ACK	ON/OFF for transmitting a ACK for receiving CAN signal with the MR8904
Terminator	ON/OFF via commands, 120 Ω ± 10 Ω built-in resistance
Baud rate	50 kbps to 1 Mbps at "High-speed", 10 kbps to 125 kbps at "Low-speed", 10 kbps to 83.3 kbps at "Single-wire"
Analyzed signal output channel	Up to 15 analog channels each equivalent to a 16-bit analog signal Up to 16 logic channels each equivalent to a 1-bit logic signal
Signal form	1-bit signal: 1 channel of Logic, or 1 channel of Analog 1-bit to 16-bits signal: 1 channel of Analog 17-bits to 32-bits signal: 2 channels of Analog * Cannot handle signals over 32-bits
ID trigger	Output "H" level pulse to designated logic channel when receiving set ID signal * Output pulse width: 50 μ s below 5 ms/div time axis, 1 sampling time at more than 10 ms/div time axis
Response time	Within 200 μ s after completely receiving CAN message
Transmit CAN message	Can transmit the setting CAN message to the CAN bus by a port

Options specifications (sold separately)

CAN Editor specifications (software bundled with the MR8904) (The following values are for one MR8904)

Operating environment	Windows 7 / Vista (32-bit/64-bit), Windows XP (32-bit)
CAN definition settings	CAN message ID, Start position, Data length Data order: U/L (Motorola), L/U (Motorola), L/U (Intel) Code: Unsigned, 1-Signed, 2-Signed
CAN db file	<ul style="list-style-type: none"> Load CAN db file Convert to ".cdf" file Register to list (editing not available), 33-bit data and above not supported Convert data order: Motorola (CANdb file) to U/L (Motorola) Convert coded file (CANdb file) to 2-Signed, IEEE float or double (CANdb file) not supported Convert signal name (CANdb file) to the label Convert comment (CANdb file) to the signal name
Registration list settings	CAN input port setting: Port 1, Port 2, Item number: 1 to 200 Setting upper / lower limit display on the MR8875 screen
CAN communication settings	<ul style="list-style-type: none"> Interface: High-speed, Low-speed, Single-wire Terminator: ON/OFF (ON is enabled at High-Speed only) ACK: ON/OFF Baud rate: AUTO (enabled at ACK OFF only) 50 kbps to 1 Mbps at "High-speed", 10 kbps to 125 kbps at "Low-speed", 10 kbps to 83.3 kbps at "Single-wire"
Analog channel settings	Number of channels: 15 <ul style="list-style-type: none"> Assign the definition on the registration list under 16-bits to 1 channel Assign the definition on the registration list for 17-bits to 32-bits to 2 channels
Logic channel settings	Number of channels: 16 <ul style="list-style-type: none"> Assign the definition on the registration list under 16-bits, with bit position Assign the definition on the registration list to the ID trigger
Transmission settings	Transmission number, Mode, CAN output port, Frame type, Transmission ID, Transmission byte length, Transmission data, Answer ID, Transmission period
Communication with the MR8875	Search MR8875 via USB, Registration list, CAN communication setting, Analog channels settings, Logic channel settings, Transmission setting information, etc.
Printing functions	Registration list, All items of CAN communication settings, Assigned analog list, Assigned logic list, All items of transmission settings
Save functions	CAN definition data: Binary form, ".cdf" extension, convertible to software for Hioki Model 8910 Setting date (All contents without CAN definition data): Binary form, ".ces" extension

Dimensions, mass: Approx. 119.5W × 18.8H × 151.5D mm (4.70W × 0.74H × 5.96D in), Approx. 185 g (6.5 oz) Accessories: None



Analog Unit MR8905 (Accuracy at 23 ± 5 °C/73 ± 9 °F, 20 to 80 % rh after 30 min. of warm-up time and zero adjustment; Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year)

Functions	No. of channels: 2, switchable between instantaneous value and AC RMS value
Input connectors	Banana connector (input impedance 4 MΩ, input capacitance less than 1 pF) Max. rated voltage to earth: CAT II 1000 V AC & DC, CAT III 600 V AC & DC (with input isolated from the main unit, the max. voltage that can be applied between input channel and chassis and between input channels without damage)
Measurement range	500 mV to 50 V/div, 7 ranges, full scale: 20 div *The maximum displayable AC voltage is 700 Vrms when using 1/2 compression of the vertical axis.
Low-pass filter	5/50/500/5 kHz, OFF
Resolution	1/1250 of measurement range (using 16-bit A/D converter)
Highest sampling rate	500 kS/s (simultaneous sampling across 2 channels)
Accuracy	±0.5% f.s. (with 5 Hz filter ON)
RMS measurement	RMS accuracy: ±1.5% f.s. (30 Hz up to but not including 1 kHz, sine wave input) or ±3% f.s. (1 kHz up to 10 kHz, sine wave input) Response time: 300 ms (filter off, rising from 0% to 90% f.s.) or 600 ms (filter off, falling from 100% to 10% f.s.) Crest factor 2
Frequency characteristics	DC to 100 kHz -3 dB
Input coupling	DC/AC-RMS/GND
Max. allowable input	1000 V DC, 700 V AC (the max. voltage that can be applied across input pins without damage)

(Compatible with MR8875 firmware version 2.14/3.14 or later)

Cable length and mass: Main unit cable 1.5 m (4.92 ft), input section cable 1 m (3.28 ft), approx. 320 g (11.3 oz)
Note: The unit-side plug of the MR9321-01 is different from the MR9321.



LOGIC PROBE MR9321-01

Function	Detection of AC or DC relay drive signal for High/Low state recording Can also be used for power line interruption detection
Input	4 channels (isolated between unit and channels), HIGH/LOW range switching Input resistance: 100 kΩ or higher (HIGH range), 30 kΩ or higher (LOW range)
Output (H) detection	170 to 250 V AC, ±DC 70 to 250 V (HIGH range) 60 to 150 V AC, ±DC 20 to 150 V (LOW range)
Output (L) detection	0 to 30 V AC, ±DC 0 to 43 V (HIGH range) 0 to 10 V AC, ±DC 0 to 15 V (LOW range)
Response time	Rising edge 1 ms max., falling edge 3 ms max. (with HIGH range at 200 V DC, LOW range at 100 V DC)
Max. allowable input	250 Vrms (HIGH range), 150 Vrms (LOW range) (the maximum voltage that can be applied across input pins without damage)

Cable length and mass: Main unit cable 1.5 m (4.92 ft), input section cable 30 cm (0.98 ft), approx. 150 g (5.3 oz)
Note: The unit-side plug of the 9320-01 is different from the 9320.



LOGIC PROBE 9320-01

Function	Detection of voltage signal or relay contact signal for High/Low state recording
Input	4 channels (common ground between unit and channels), digital/contact input, switchable (contact input can detect open-collector signals) Input resistance: 1 MΩ (with digital input, 0 to +5 V) 500 kΩ or more (with digital input, +5 to +50V) Pull-up resistance: 2 kΩ (contact input: internally pulled up to +5 V)
Digital input threshold	1.4V/ 2.5V/ 4.0V
Contact input detection resistance	1.4 V: 1.5 kΩ or higher (open) and 500 Ω or lower (short) 2.5 V: 3.5 kΩ or higher (open) and 1.5 kΩ or lower (short) 4.0 V: 25 kΩ or higher (open) and 8 kΩ or lower (short)
Response speed	500 ns or lower
Max. allowable input	0 to +50 V DC (the maximum voltage that can be applied across input pins without damage)



Cable length and mass: 70 cm (2.30 ft), Output side: 1.5 m (4.92 ft), 170g (6.0 oz)

DIFFERENTIAL PROBE P9000 (Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year)

Measurement modes	P9000-01: For waveform monitor output, Frequency properties: DC to 100 kHz -3 dB P9000-02: Switches between waveform monitor output/AC effective value output Wave mode frequency properties: DC to 100 kHz -3 dB, RMS mode frequency properties: 30 Hz to 10 kHz, Response time: Rise 300 ms, Fall 600 ms
Division ratio	Switches between 1000:1, 100:1
DC output accuracy	±0.5 % f.s. (f.s. = 1.0 V, division ratio 1000:1), (f.s. = 3.5 V, division ratio 100:1)
Effective value measurement accuracy	±1 % f.s. (30 Hz to less than 1 kHz, sine wave), ±3 % f.s. (1 kHz to 10 kHz, sine wave)
Input resistance/capacity	H-L: 10.5 MΩ, 5 pF or less (at 100 kHz)
Maximum input voltage	1000 V AC, DC
Maximum rated voltage to ground	1000 V AC, DC (CAT III)
Operating temperature range	-40°C to 80°C (-40°F to 176°F)
Power supply	(1) AC adapter Z1008 (100 to 240 V AC, 50/60 Hz), 6 VA (including AC adapter), 0.9 VA (main unit only) (2) USB bus power (5 V DC, USB-microB terminal), 0.8 VA (3) External power source 2.7 V to 15 V DC, 1 VA
Accessories	Instruction manual ×1, Alligator clip ×2, Carrying case ×1


Capture Voltage Signals from Outside the Wire Cover: SP3000-01

Measure signals from electric equipment on vehicles, capture LIN and other communications signals.

- Measure insulated wires with outside diameters 1 mm to 2.5 mm
- 10 Hz to 100 kHz band width

Analyzing data on a computer

- **WAVE PROCESSOR 9335 (option)**
 - Waveform display and calculation
 - Print function
- **Wave Viewer (Wv) Software (bundled software)**
 - Confirmation of binary data waveforms on a computer
 - Saving data in the CSV format for transfer to spreadsheet software



9335 Outline specifications (option)

Operating environment	Windows 10/8/7 (32/64-bit), Vista (32-bit), XP
Functions	<ul style="list-style-type: none"> Display: Waveform display, X-Y display, cursor function, etc. File loading: Readable data formats (.MEM, .REC, .RMS, .POW) Largest readable file: Largest file that can be saved by supported instruments (Supported file size may be limited due to computer's operating environment.) Data conversion: Conversion to CSV format, batch conversion of multiple files
Print	<ul style="list-style-type: none"> Print function: Saving of print image files (with support for enhanced metafile [EMF] format) Print format: Select from no tiling, 2 to 16 tiles, 2 to 16 rows, X/Y 1 to 4 tiles, preview/hard copy

Wave Viewer (Wv) Outline specifications (bundled software)

Operating environment	Windows 10/8/7 (32/64-bit), Vista (32-bit), XP
Functions	<ul style="list-style-type: none"> Simple display of waveform file Convert binary data file to text format, CSV Scroll display, enlarge/reduce, jump to cursor/trigger position, etc.

MR8875 Options in Detail

*Install by inserting into the main unit. Can be replaced by user. Input cables are not supplied.

Input modules

- ANALOG UNIT MR8901**
4ch, Voltage measurement, DC to 100kHz bandwidth
- VOLTAGE/TEMP UNIT MR8902**
15ch, Voltage measurement, Thermocouple measurement
- STRAIN UNIT MR8903**
4ch, Voltage measurement, Strain gauge converter input, Conversion cable included
- CAN UNIT MR8904**
Up to 15 analog channels each equivalent to a 16-bit analog signal, and up to 16 logic channels each equivalent to a 1-bit logic signal
- ANALOG UNIT MR8905**
2 channels, high-voltage DC/RMS input, DC to 100 kHz band
(Compatible with MR8875 firmware version 2.14/3.14 or later)

*Voltage is limited to the specifications of the input modules in use

- ALLIGATOR CLIP L9790-01**
Red/black set attaches to the ends of the cables L9790
- CONTACT PIN 9790-03**
Red/black set attaches to the ends of the cables L9790
- GRABBER CLIP 9790-02**
Red/black set attaches to the ends of the cables L9790
- CONNECTION CORD L9790**
Flexible ϕ 4.1 mm (0.16 in) thin dia., cable allowing for up to 600 V input. 1.8 m (5.91 ft) length
* The end clip is sold separately.

*Voltage is limited to the specifications of the input modules in use

- CONNECTION CORD L9198**
 ϕ 5.0 mm (0.20 in) dia., cable allowing for up to 300 V input. 1.7 m (5.58 ft) length, small alligator clip

* Voltage input via banana terminals limited by the voltage specifications of the respective input unit.

- CONNECTION CABLE SET L4940**
Banana plug - banana plug, 1.5 m (4.92 ft) length, red/black each 1
- EXTENSION CABLE L4931**
Expands the length of the cable with banana plug, 1.5 m (4.92 ft) length
- ALLIGATOR CLIP L4935**
Attaches to the tip of the banana plug cable, CAT IV 600V, CAT III 1000V
- BUS BAR CLIP L4936**
Attaches to the tip of the banana plug cable, CAT III 600V
- MAGNETIC ADAPTER L4937**
Attaches to the tip of the banana plug cable, CAT III 1000V
- GRABBER CLIP 9243**
Attaches to the tip of the connection cable, 1.96 mm (7.72 in) length, CAT III 1000 V

*Voltage to ground is within this product's specifications. Separate power source is also required.

- DIFFERENTIAL PROBE P9000-01**
Waveform only, up to 1 kV AC/DC, band width up to 100kHz
- DIFFERENTIAL PROBE P9000-02**
Waveform/RMS value switchable, up to 1 kV AC/DC, band width up to 100kHz
- AC ADAPTER Z1008**
100 to 240 V AC

*For P9000. Inquire with your Hioki distributor.

- (1) Bus powered USB cable
- (2) USB(A) - Micro B cable
- (3) 3-prong cable

Other options for Input

- CONNECTION CORD L9217**
Cord has insulated BNC connectors at both ends, 1.6 m (5.25 ft) length
- CONVERSION ADAPTER 9199**
Receiving side banana, output BNC terminal
- CAN CABLE 9713-01**
For the MR8904(MR8875), 8910, Unprocessed on one end, 1.8 m (5.91 ft) length

*For reference only. Please purchase locally.

- Thermocouple**



Model : MEMORY HiCORDER MR8875

Model No.(Order Code) (Note)

MR8875 (Max. 16 - 60ch, 32MW memory, main unit only)

*Cannot operate alone, You must install other options

* Only the small terminal types can be used. * The 9323 is not required for the small-terminal types 9327, 9320-01, 9321-01 and MR9321-01.

- LOGIC PROBE 9320-01**
4-channel type, for voltage/contact signal ON/OFF detection (response pulse width 500 ns or more, miniature terminal type)
- LOGIC PROBE MR9321-01**
4 isolated channels, ON/OFF detection of AC/DC voltage (miniature terminal type)
- CONVERSION CABLE 9323**
*Used for connecting the 9320/9321/MR9321 and the 9324 to the Memory HiCorder with small logic terminal models

- SD MEMORY CARD 2GB Z4001**
2GB capacity
- SD MEMORY CARD Z4003**
8 GB capacity
- SD Card Precaution**
Use only SD Cards sold by HIOKI. Compatibility and performance are not guaranteed for SD cards made by other manufacturers. You may be unable to read from or save data to such cards.

- WAVE PROCESSOR 9335**
Convert data, print and display waveforms
- LAN CABLE 9642**
Straight Ethernet cable, supplied with straight to cross conversion cable, 5 m (16.41 ft) length

- DIFFERENTIAL PROBE 9322**
For up to 1kV AC or 2kV DC, frequency band width up to 10MHz
- AC ADAPTER 9418-15**
100 to 240 V AC.

- AC ADAPTER Z1002**
For main unit, 100 to 240 V AC
- BATTERY PACK Z1003**
NiMH, Charges while installed in the main unit

- CARRYING CASE C1004**
Includes compartment for options, hard trunk type, also suitable for transporting the MR8875

*A separate power supply (CT955x) is required in order to use a high-precision current sensor.
*Only sensors with ME15W (12-pin) terminals (-05 type) can be connected to the CT955x.
*The separately available Conversion Cable CT9900 is required in order to use a sensor with PL23 (10-pin) terminal.

- POWER SUPPLY for Current Sensors**
SENSOR UNIT CT9555 1ch, with Waveform output
CONNECTION CORD L9217
Cord has insulated BNC connectors at both ends, 1.6 m (5.25 ft) length
- PL23 (10-pin) - ME15W (12-pin) conversion**
CONVERSION CABLE CT9900
Convert PL23 (10-pin) terminal to ME15W (12-pin) terminal
- Up to 1000 A (High precision) *ME15W (12-pin) terminal type**
High-precision pull-through type, monitor the waveforms of DC to distorted AC current
AC/DC CURRENT SENSOR 9709-05, 100 kHz band width, 500A
Monitor the waveforms of DC to distorted AC current
AC/DC CURRENT PROBE CT6844-05, 200 kHz band width, 500A
AC/DC CURRENT PROBE CT6845-05, 100 kHz band width, 500A
AC/DC CURRENT PROBE CT6846-05, 20 kHz band width, 1000A

Precautions when connecting a high-precision current sensor to a Memory HiCorder
Connecting to the MR8880/MR8875/MR8870
• High-precision current sensor (ME15W) + CT9555 + BNC cable → MR8875
• High-precision current sensor (PL23) + CT9900 + CT9555 + BNC cable → MR8875

Other current sensor types
The MR8875 can be used with various types of current sensors and probes. For details, see product information on Hioki's website.

- The CT7290 (available separately) is required in order to use these current sensors
- 100 A to 2000 A (Medium speed)**
AC/DC CURRENT SENSOR CT7631, (Auto zero CT7731)
DC, 1 Hz to 10 kHz (-3dB), 100 A, 1 mV/A output
- AC/DC CURRENT SENSOR CT7636**, (Auto zero CT7736)
DC, 1 Hz to 10 kHz (-3dB), 600 A, 1 mV/A output
- AC/DC CURRENT SENSOR CT7642**, (Auto zero CT7742)
DC, 1 Hz to 10 kHz (5 kHz), 2000 A, 1 mV/A output
- DISPLAY UNIT CM7290**
Provides measurement, display, and output functionality when used with the CT7000s.
- DISPLAY UNIT CM7291**
with built-in Bluetooth® wireless technology
- OUTPUT CORD L9095**
Connect to BNC terminal, 1.5 m (4.92 ft) length

- 500 A to 5000 A *For commercial power lines, 50/60 Hz**
CLAMP ON PROBE 9018-50
Good phase characteristics, Frequency characteristics: 40 Hz to 3 kHz, 10 to 500 A AC range, output 0.2 V AC f.s.
- CLAMP ON PROBE 9132-50**
Frequency characteristics: 40 Hz to 1 kHz, 20 to 1000 A AC range, output 0.2 V AC f.s.
- AC FLEXIBLE CURRENT SENSOR CT9667-01/-02/-03**
10 Hz to 20 kHz, 5000 A / 500 A AC, 500 mV/f.s. output, ϕ 100 to 254 mm (3.94 to 10.00 in), 3 loop diameters

- Leak Current *For commercial power lines, 50/60 Hz**
CLAMP ON LEAK HITESTER 3283
10 mA range / 10 μ A resolution to 200 A range, with monitor/analog output 1 V f.s.
- OUTPUT CORD L9095**
Connect to BNC terminal, 1.5 m (4.92 ft) length
- AC ADAPTER 9445-02**
For USA, 100 to 240 V AC, 9 V / 1 A
- AC ADAPTER 9445-03**
For EU 100 to 240 V AC, 9 V / 1 A

- NON-CONTACT AC VOLTAGE PROBE SP3000-01**
5 Vrms rated, 10 Hz to 100 kHz band width
- NON-CONTACT AC VOLTAGE PROBE SP3000**
Sold individually
- AC VOLTAGE PROBE SP9001**
Sold individually

Note: Company names and Product names appearing in this catalog are trademarks or registered trademarks of various companies.

HIOKI

HIOKI E. E. CORPORATION

HEADQUARTERS

81 Koizumi, Ueda, Nagano, 386-1192, Japan
TEL +81-268-28-0562 FAX +81-268-28-0568
http://www.hioki.com / E-mail: os-com@hioki.co.jp

HIOKI USA CORPORATION

TEL +1-609-409-9109 FAX +1-609-409-9108
http://www.hiokiusa.com / E-mail: hioki@hiokiusa.com

HIOKI (Shanghai) SALES & TRADING CO., LTD.
TEL +86-21-63910090 FAX +86-21-63910360
http://www.hioki.cn / E-mail: info@hioki.com.cn

HIOKI SINGAPORE PTE. LTD.
TEL +65-6634-7677 FAX +65-6634-7477
E-mail: info-sg@hioki.com.sg

HIOKI KOREA CO., LTD.
TEL +82-2-2183-8847 FAX +82-2-2183-3360
E-mail: info-kr@hioki.co.jp

DISTRIBUTED BY